

Accuracy of CAD Models of the Jaws Produced Using Ultra-low MDCT Doses and ASIR and MBIR

International Journal of Computer Assisted Radiology and Surgery

Asma'a A. Al-Ekrish (corresponding author), BDS, MDS, Cert. Diag. Sci.

King Saud University, Department of Oral Medicine and Diagnostic Sciences

E-mail: aalekrish@ksu.edu.sa; asma.alekrish@gmail.com

Sara A. Alfadda, BDS, MSc, PhD, FRCD(C),

Wadea Ameen, MSC, PhD candidate

Romed Hörmann, Research Assistant

Wolfgang Puelacher, MD, DMD

Gerlig Widmann, MD, EBIR

Electronic supplementary material 2. Color coded analysis demonstrating the location, magnitude and direction of the deviations between each test model and the reference model (in mm) (see color scale on the side).





Filtered Backprojection

ASIR 50





ASIR 100

MBIR





Test protocol 1

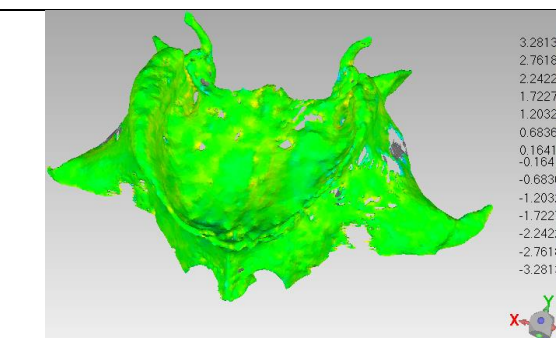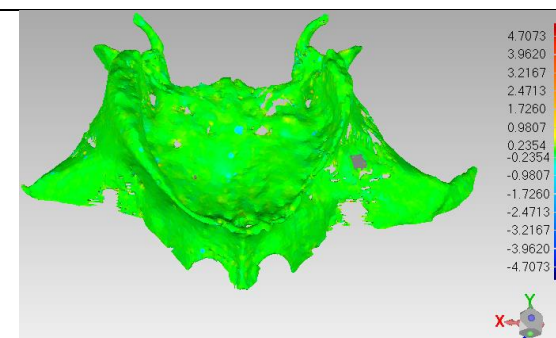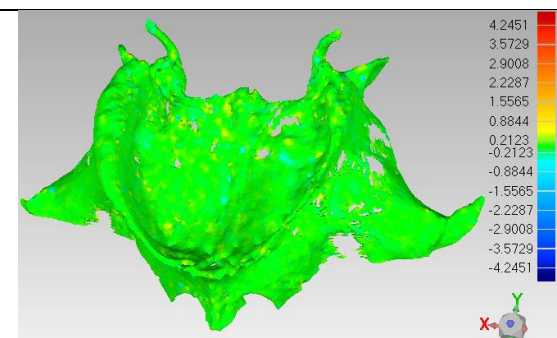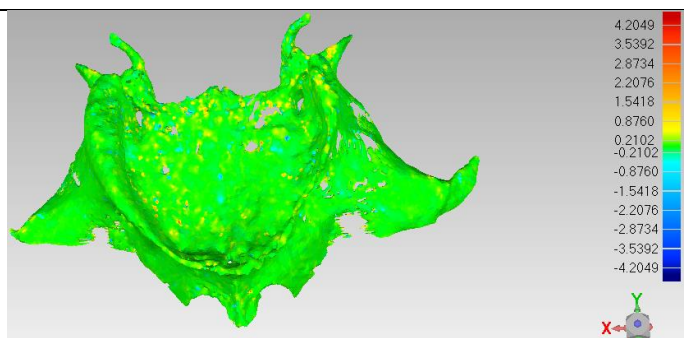





Test protocol 2

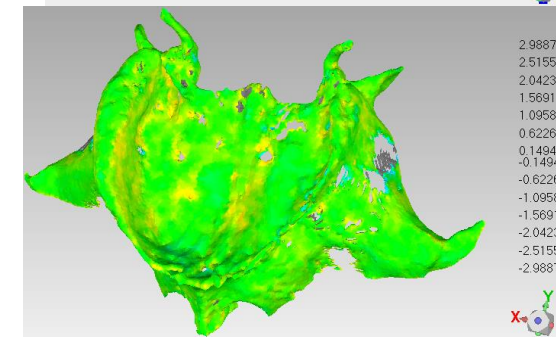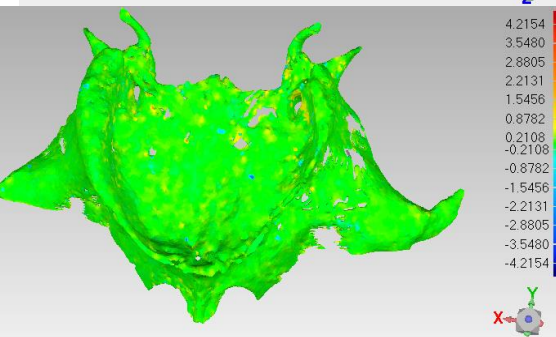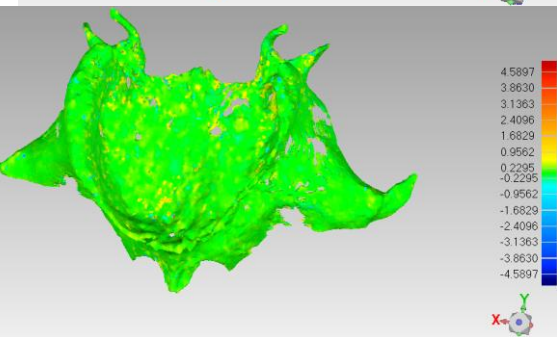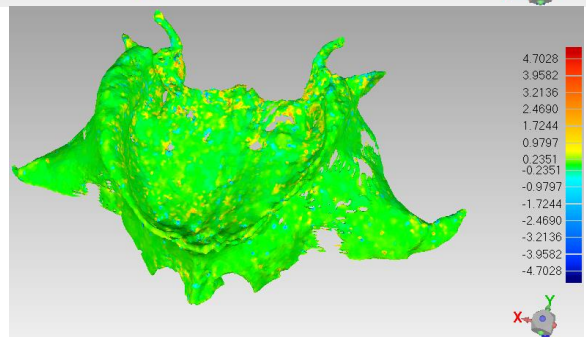

Test protocol 3

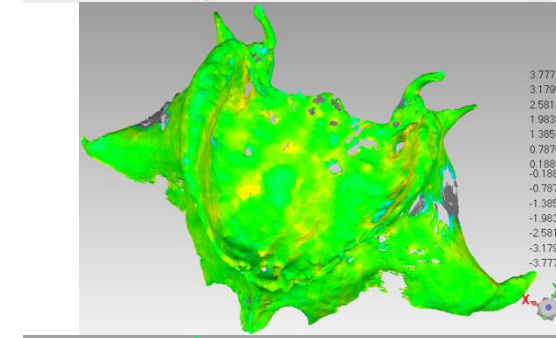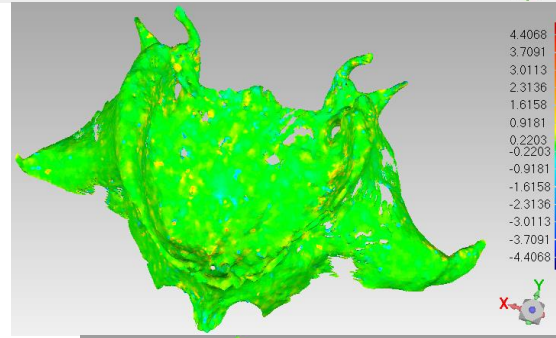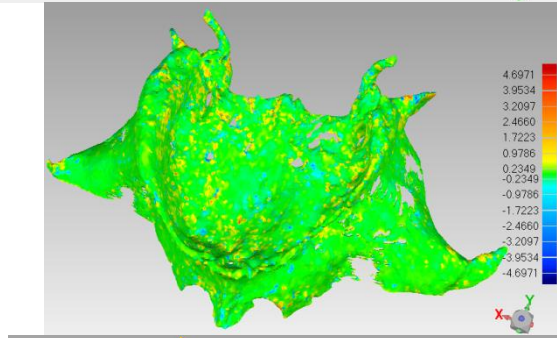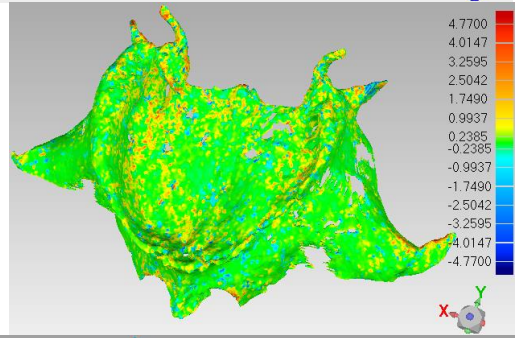

Test protocol 4

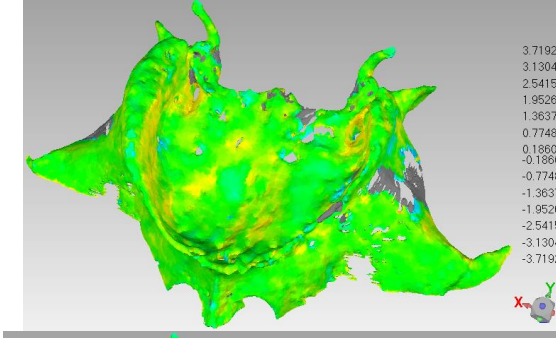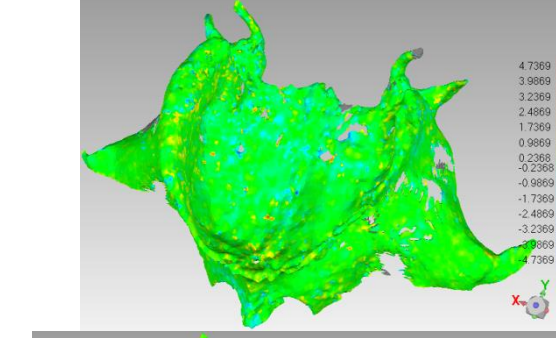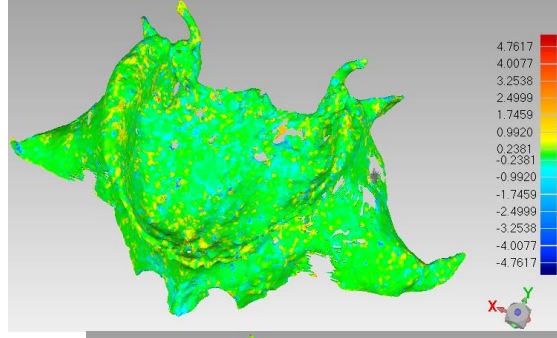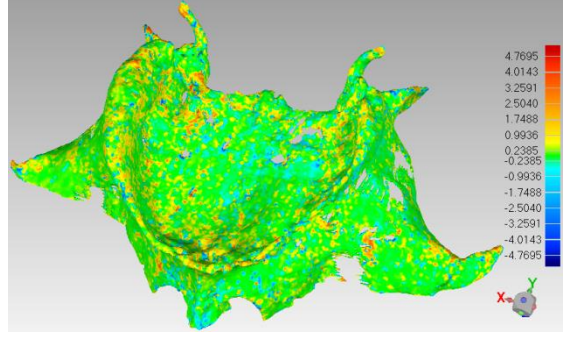

Test protocol 5

Analysis not performed due to inability to segment the maxilla.

