

Online Resource 6

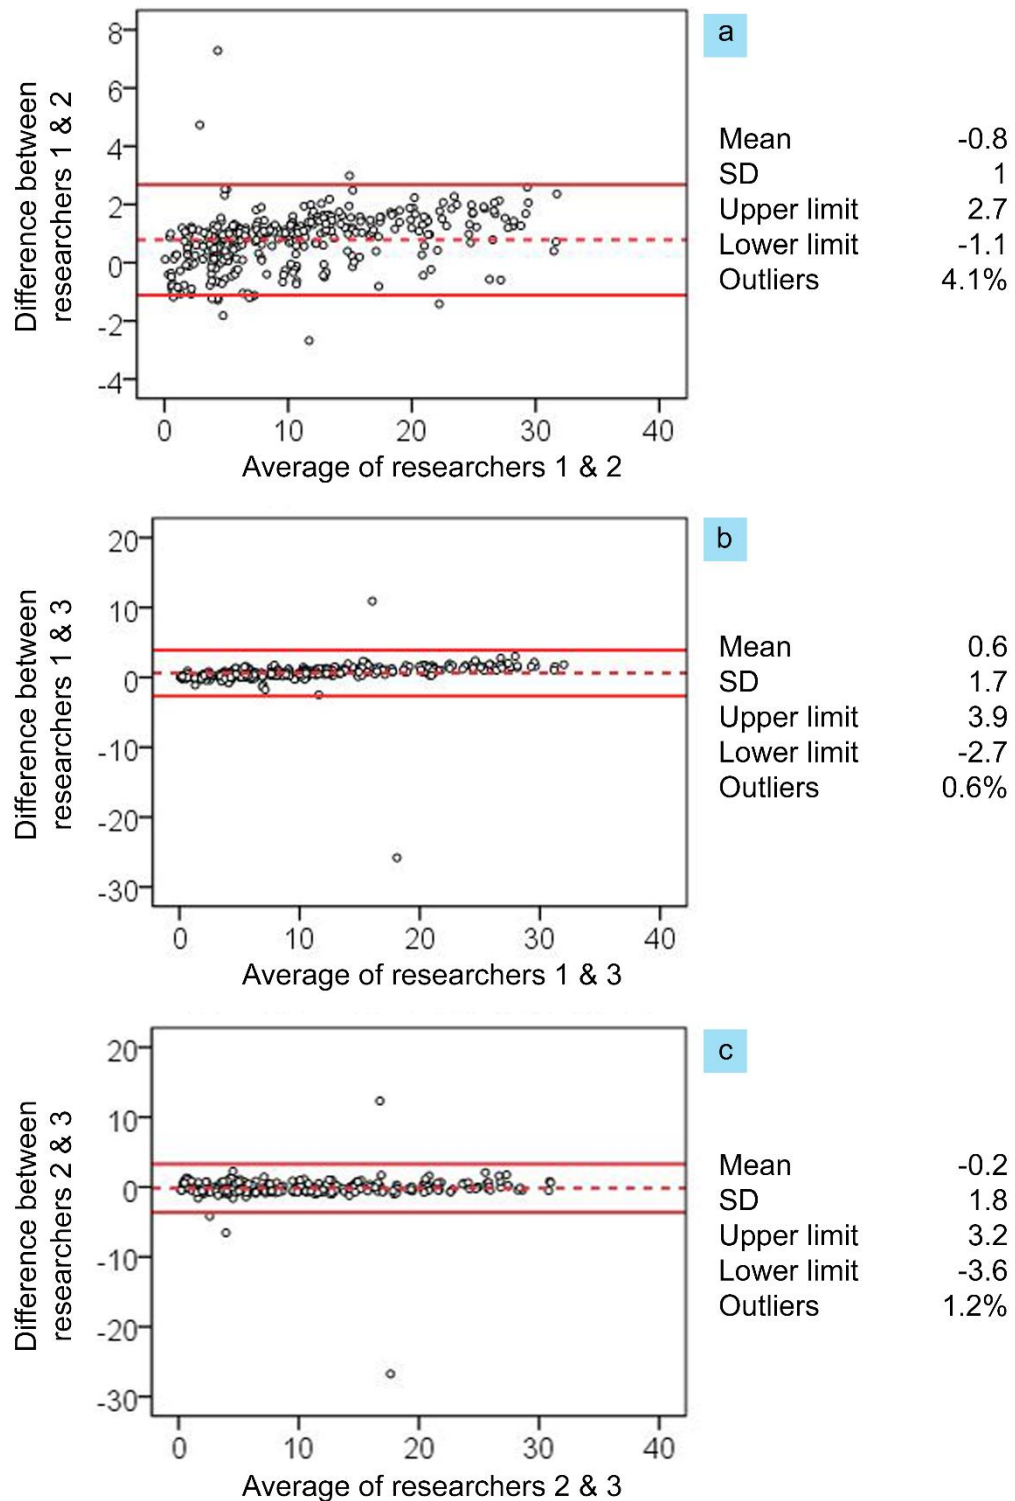


Fig. S5 Inter-observer error in the measurement of distance-to-monitor for researchers 1 and 2 (a), 1 and 3 (b), and 3 and 2 (c)

Title: Effect of marker position and size on the registration accuracy of HoloLens in a non-clinical setting with implications for high-precision surgical tasks

Journal: International Journal of Computer Assisted Radiology and Surgery

Authors: Laura Pérez-Pachón¹, Parivrudh Sharma¹, Helena Brech¹, Jenny Gregory¹, Terry Lowe^{1,3}, Matthieu Poyade², Flora Gröning¹

¹ School of Medicine, Medical Sciences and Nutrition, University of Aberdeen, Aberdeen, United Kingdom

² School of Simulation and Visualisation, Glasgow School of Art, Glasgow, United Kingdom

³ Head and Neck Oncology Unit, Aberdeen Royal Infirmary (NHS Grampian), Aberdeen, United Kingdom

Corresponding author: laura.perezpachon@gmail.com (LP)